

Quality Lab Accessories L.L.C


100 Emlen Way Suite 108 – Telford, PA. 18969

Tel. (908) 685-7500 Fax. (908) 526-4151

Certificate of Analysis

Part Number	Part Description	Serial Numbers
BSK040-01	40 Mesh Basket Assembly, Vankel	QA66303

Quality Lab Accessories L.L.C Certifies, Warrants and Represents that the items described herein conform to the specifications set forth in U.S. Pharmacopoeia, General Chapter, (711) Dissolution as last revised, as well as ASTM E 2503-07 and that all components of the listed part number this represents were designed, manufactured or fabricated within strict compliance of these same standards.

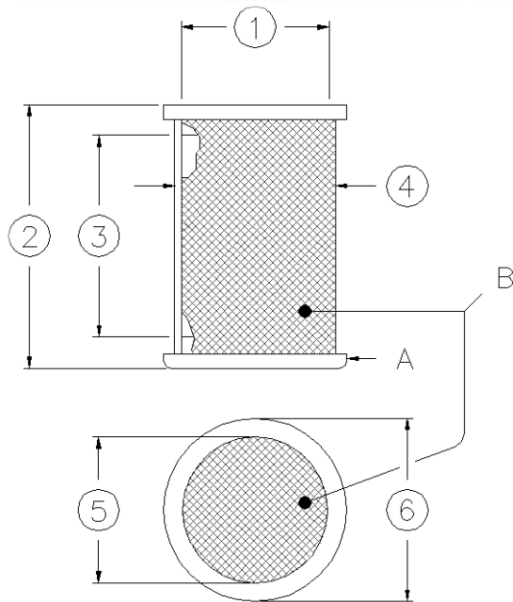

No.	USP	QLA
1	Clear Opening 20.2 +/- 1.0 MM	20.21mm
2	37.0 +/- 3.0 MM	36.47mm
3	27.0 +/- 1.0 MM Open Screen	26.41mm
4	Screen O.D. 22.2 +/- 1.0 MM	22.35mm
5	20.2 +/- 1.0 MM	20.20mm
6	25.0 +/- 3.0 MM	25.40mm
A	Maximum allowable run -out is +/- 1.0 mm	0.063mm
B	0.25 - 0.31 mm wire diameter with wire openings of 0.36-0.44 mm	0.25mm Wire/ 0.38mm Opening

Material
316L Stainless Steel

Gregory D. Matherly

Certified By

Signature

12/16/2013

Date